

FIG. 1

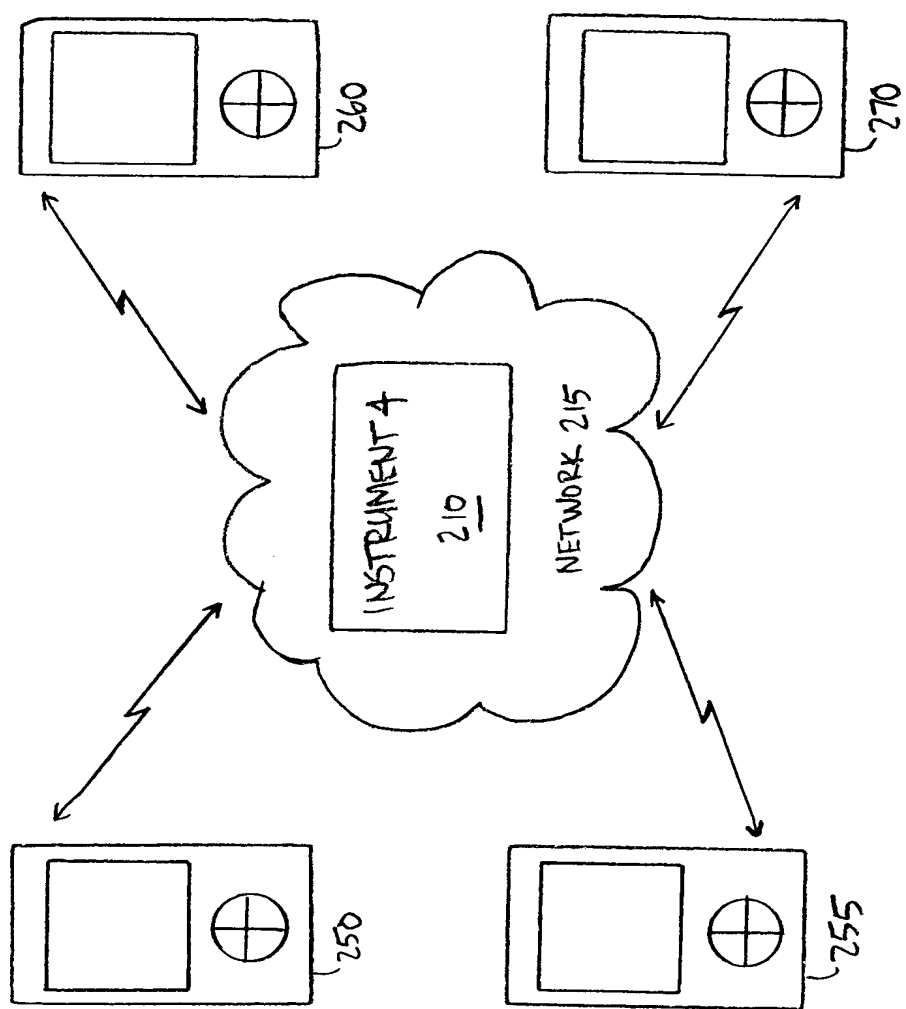


FIG. 2

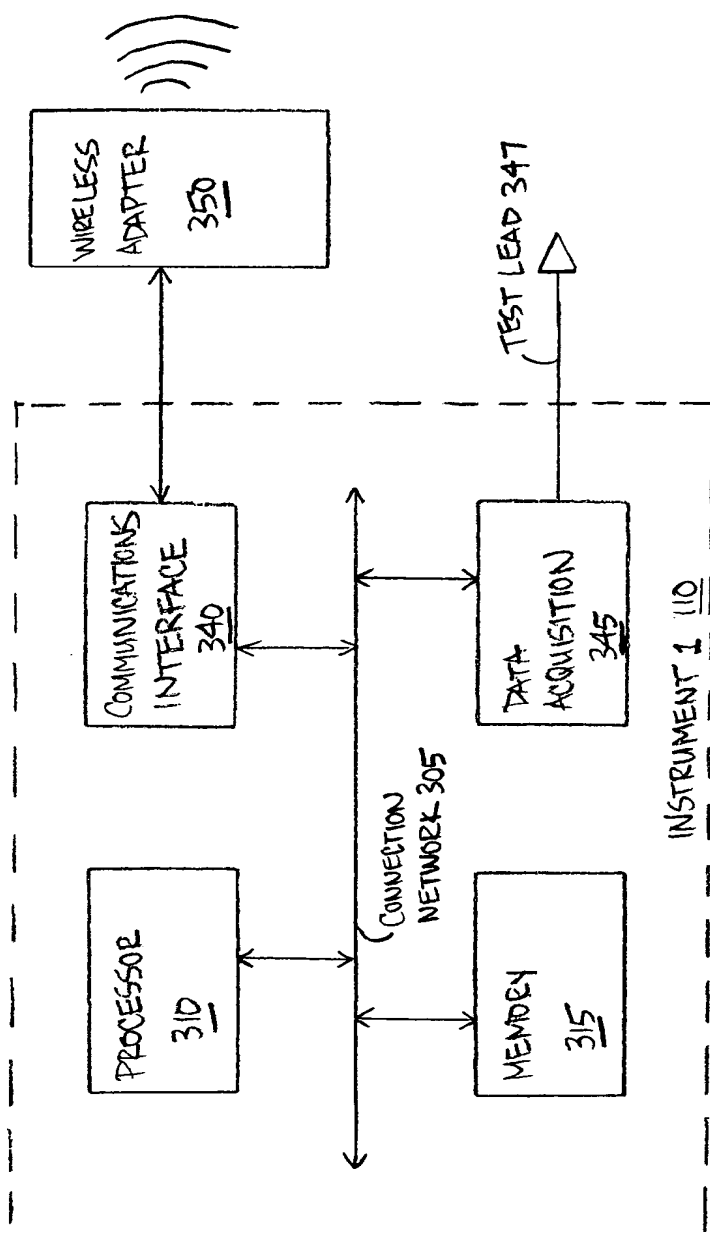


FIG. 3

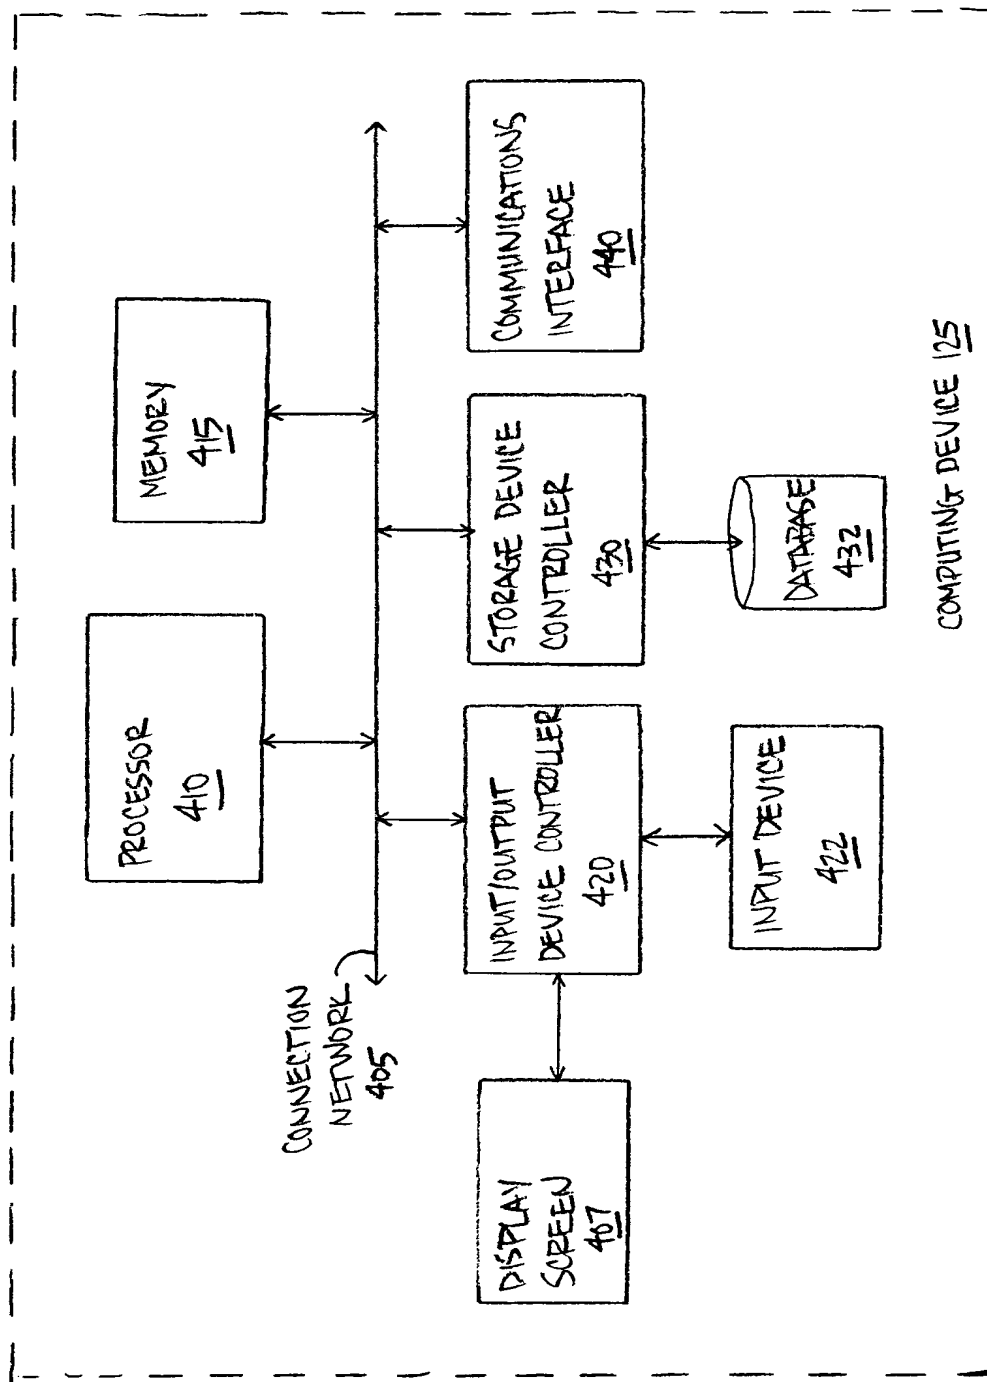


FIG. 4

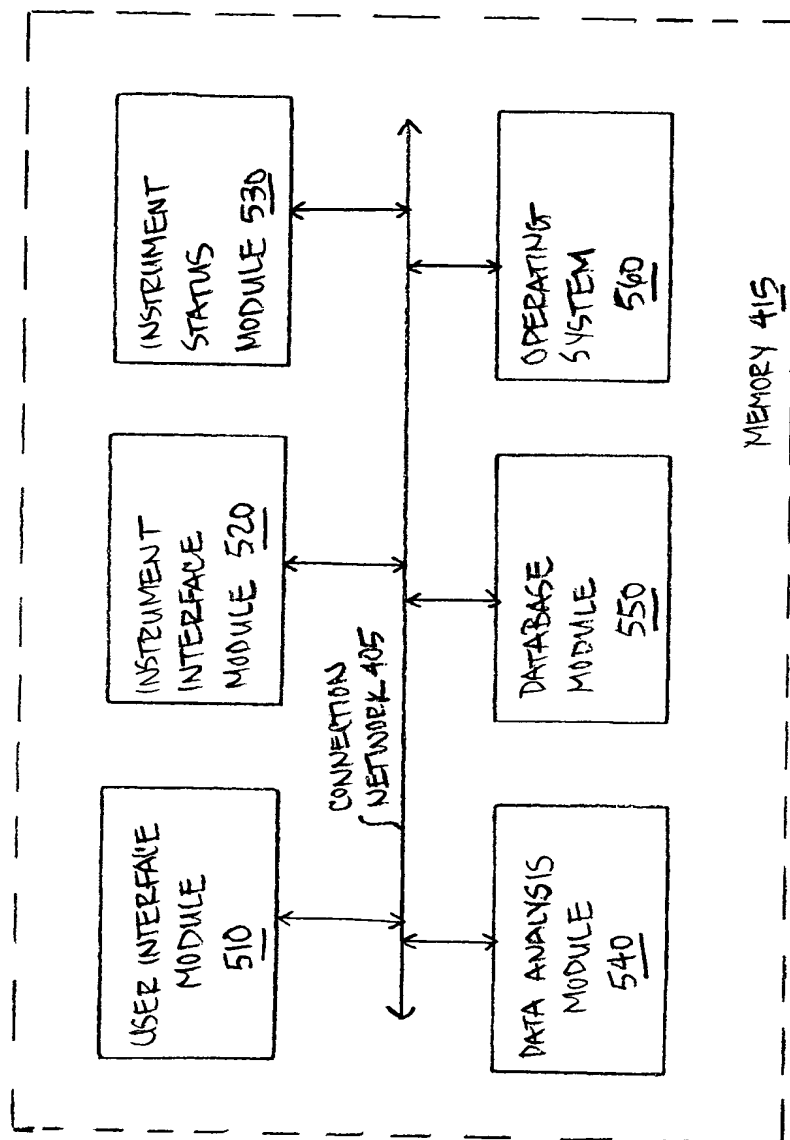


FIG. 5

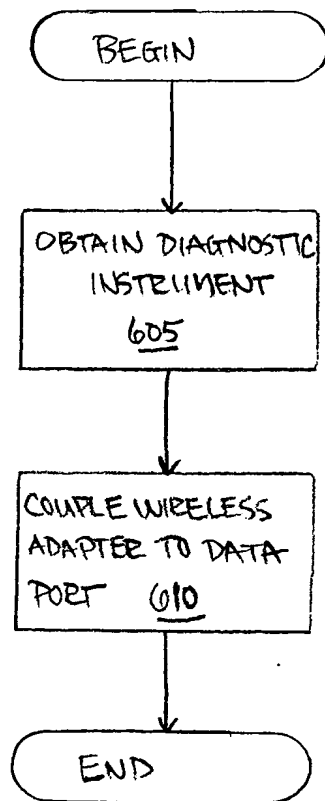


FIG. 6

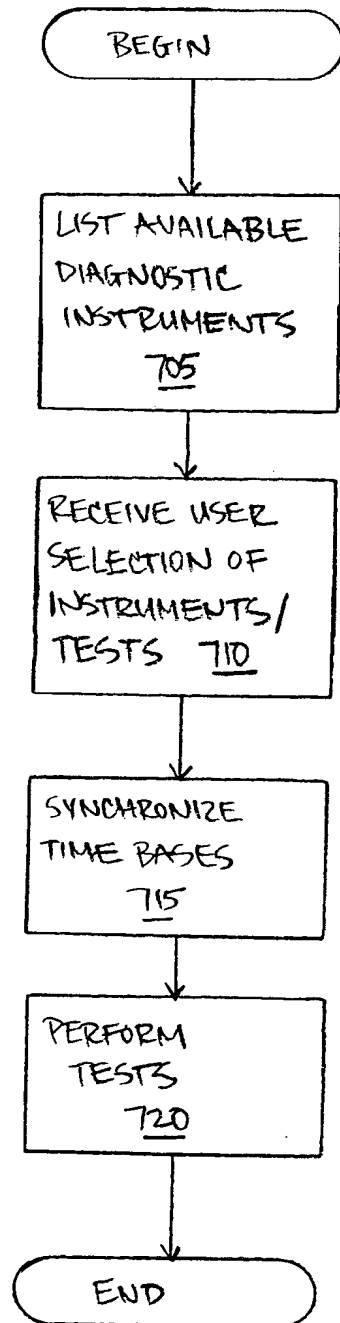


FIG. 7

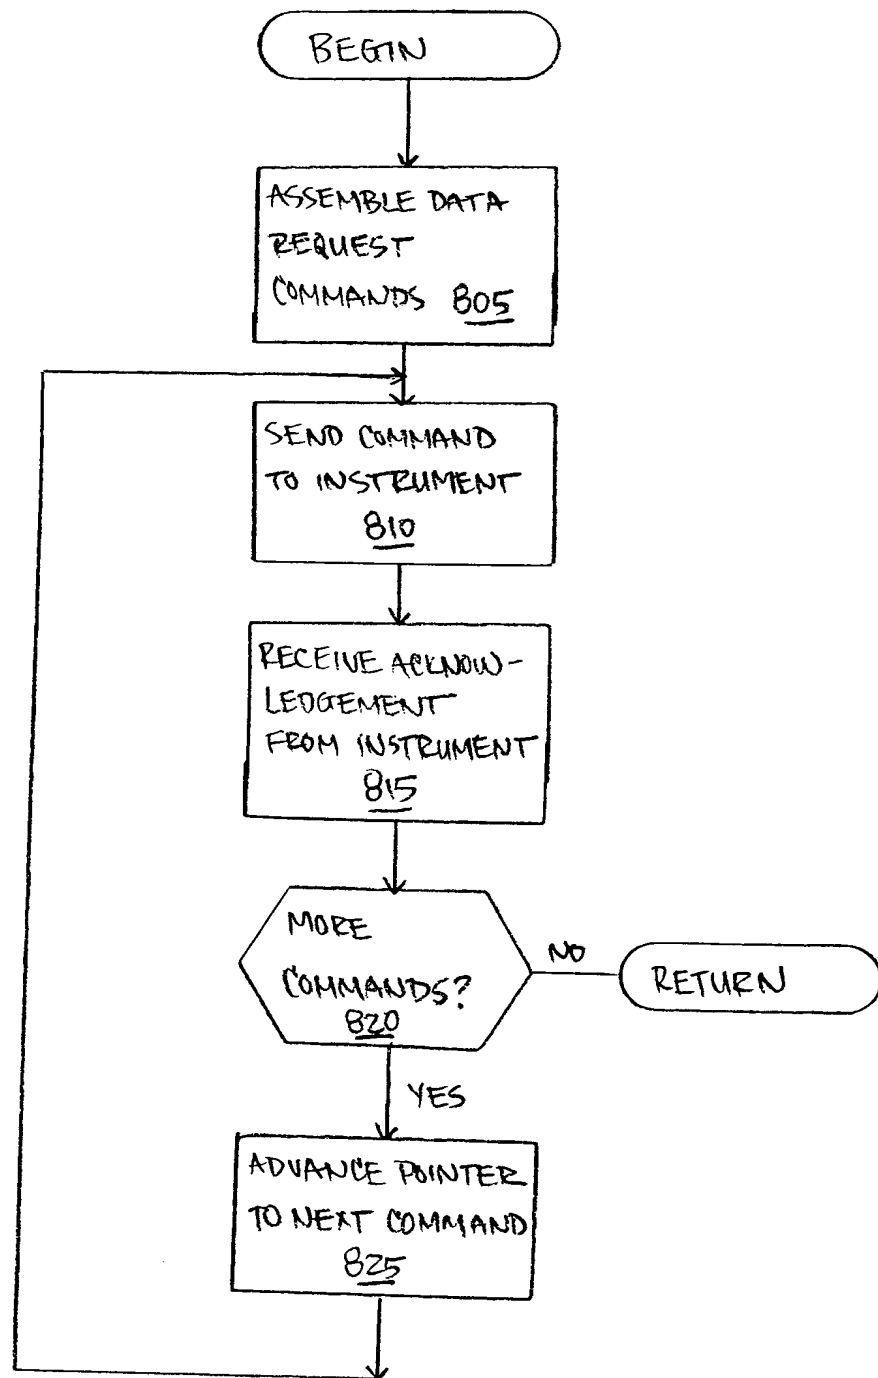


FIG. 8

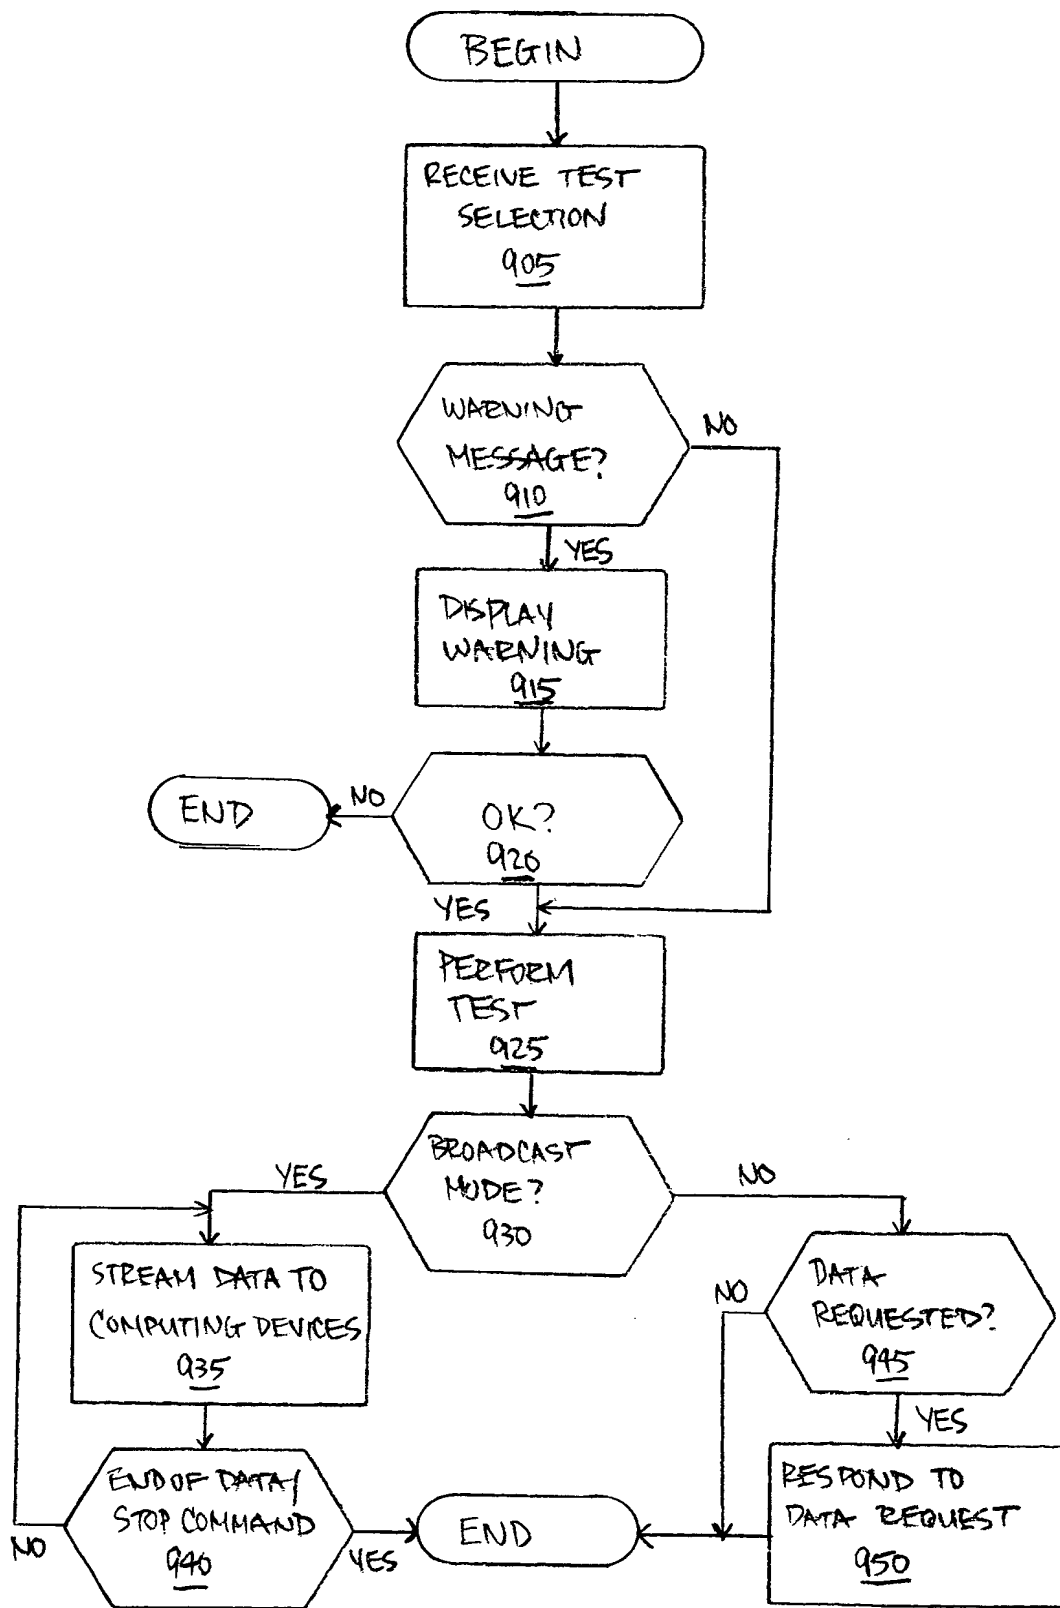


FIG. 9

AVAILABLE DIAGNOSTIC INSTRUMENTS			
§ 1005 INSTRUMENT	§ 1010 ACTIVE	§ 1015 MASTER MODE	§ 1020 BROADCAST MODE
INSTRUMENT 1	<input checked="" type="checkbox"/>	<input checked="" type="checkbox"/>	<input type="checkbox"/>
INSTRUMENT 2	<input checked="" type="checkbox"/>	<input type="checkbox"/>	<input checked="" type="checkbox"/>
INSTRUMENT 3	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
INSTRUMENT 4	<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
<div>OK 1050</div>			

DISPLAY SCREEN 407

FIG. 10

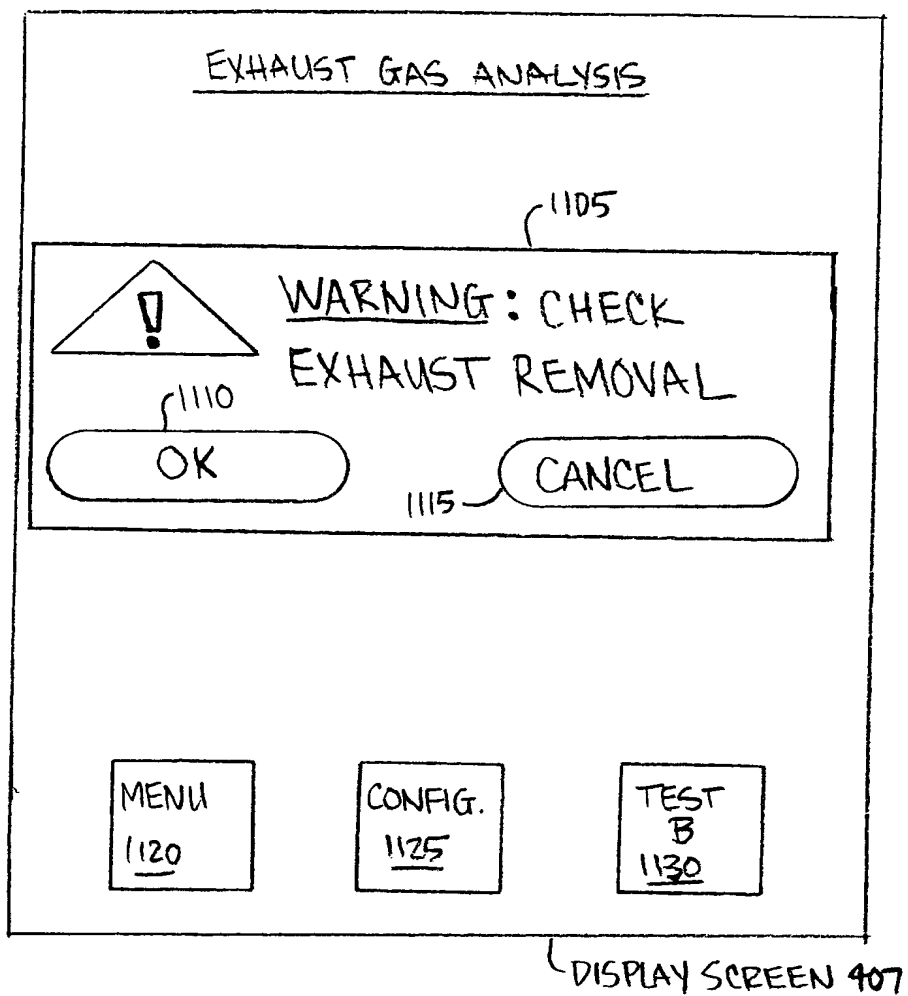


FIG. 11